



May14, 2014 3-laser 8 color (4-2-2)

Cytometer:	FACSCantoII	User:	Administrator
Cytometer Name:	FACSCantoII	Institution:	FOMD
Serial Number:	V96100493	Software:	BD FACSDiva 6.1.3
Input Device:	Carousel	Date:	1/22/2015 9:40:22 AM
Window Extension:	7.00		


Blue Laser
(488nm)
FSC

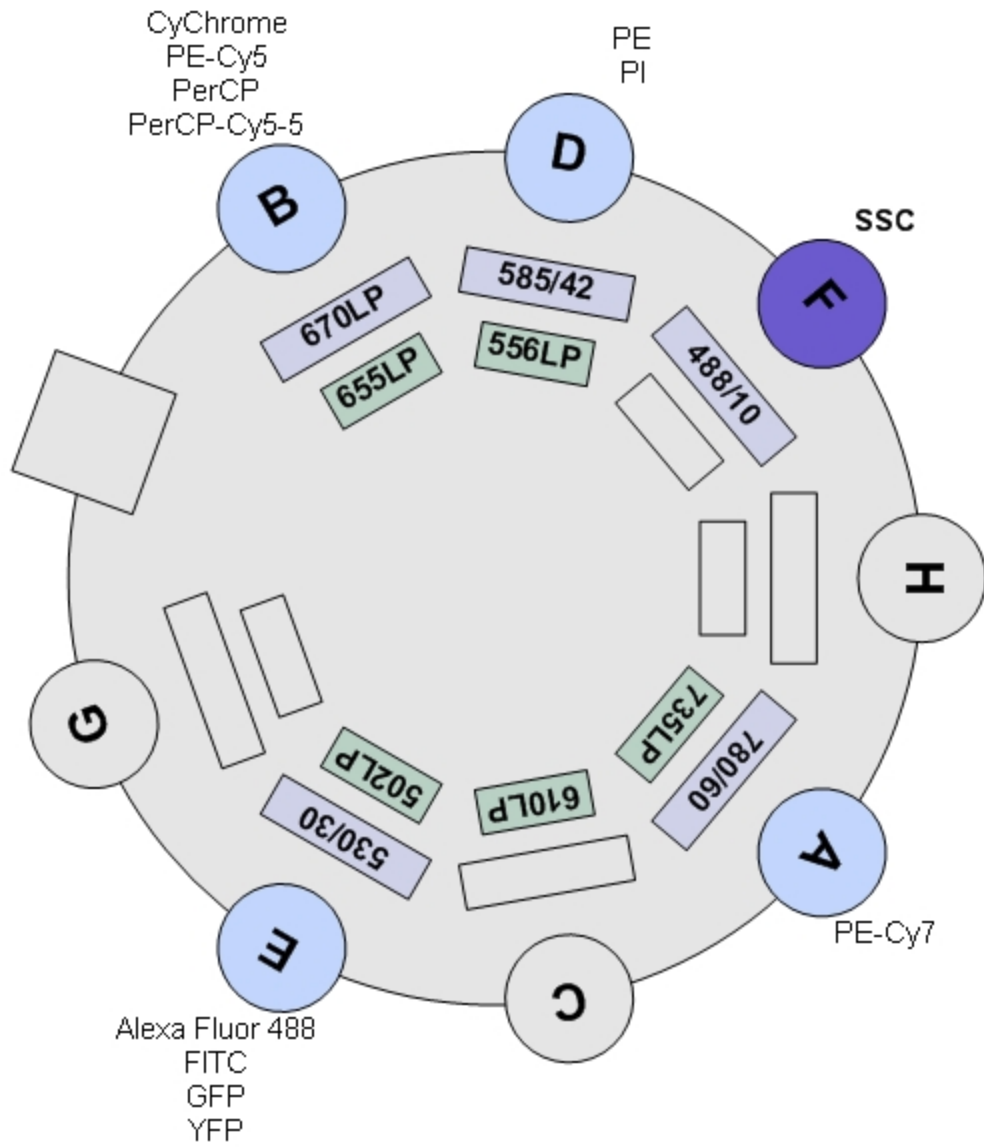

Red Laser
(633nm)

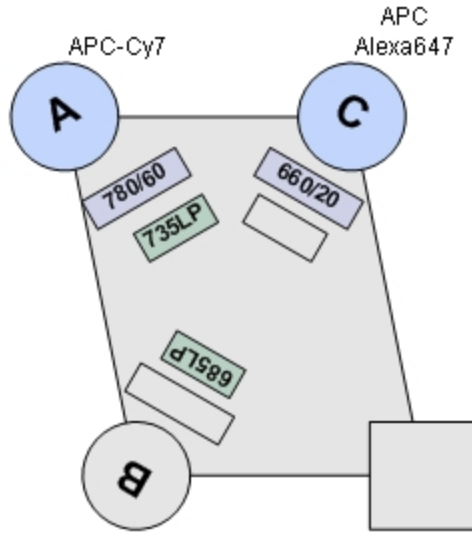

Violet Laser
(405nm)

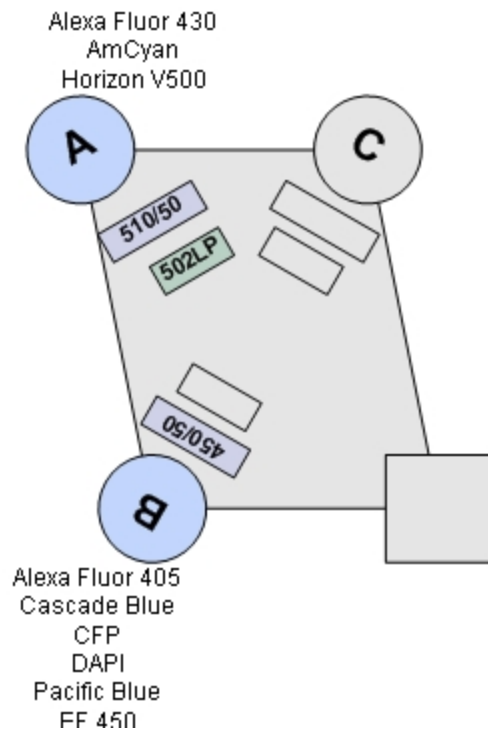

Comments: