



1Blue 3- Red 2- Violet 6- YG 4 - 70um

Cytometer:	FACSriaII	User:	Administrator
Cytometer Name:	FACSriaII	Institution:	
Serial Number:	P0088	Software:	BD FACSDiva 6.1.3
Input Device:	Manual	Date:	2/10/2015 10:31:47 AM
Sheath Pressure:	70.00		
Nozzle Size:	70		
Window Extension:	2.00		


40011111 Laser
(488nm)
ESC

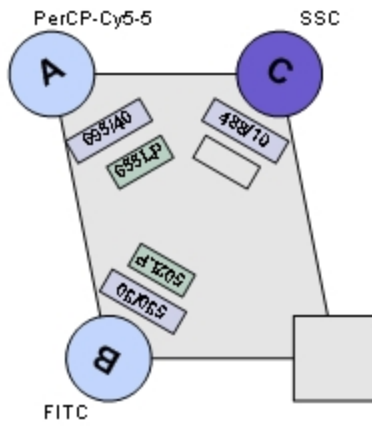


561nm Laser
(561nm)

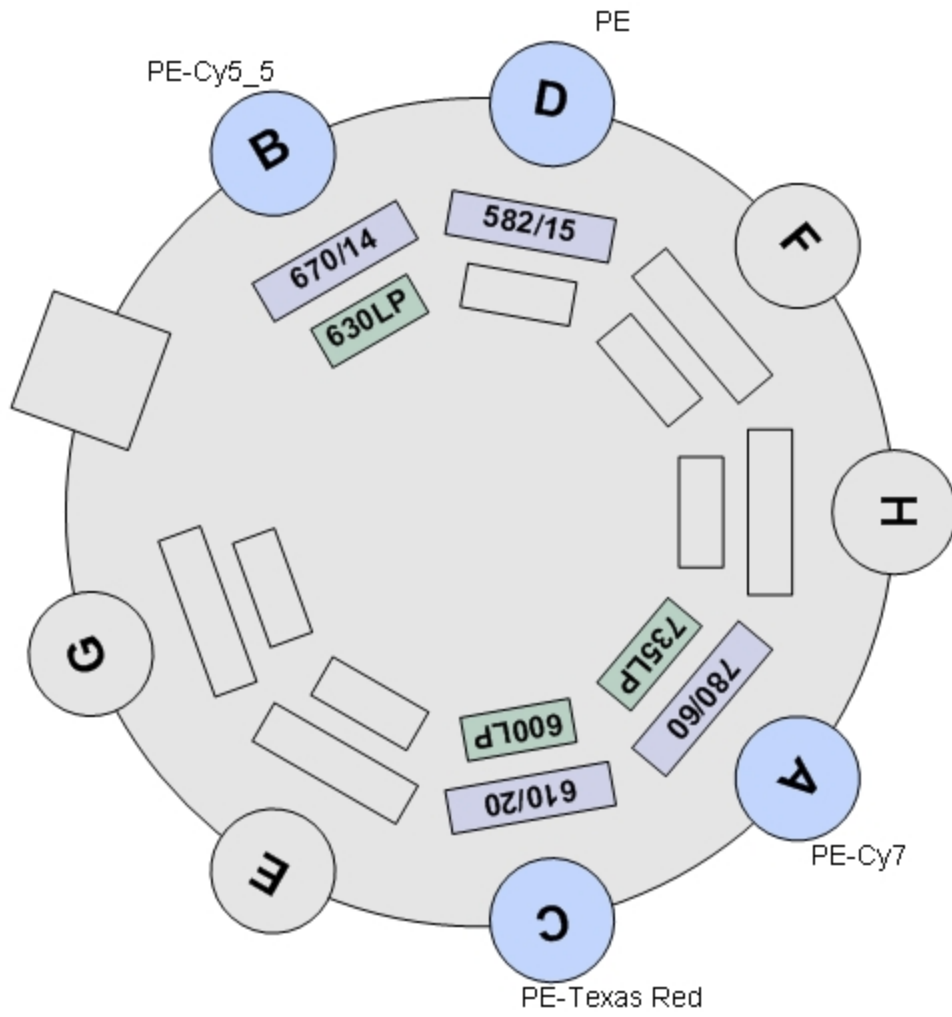

633nm Laser
(633nm)

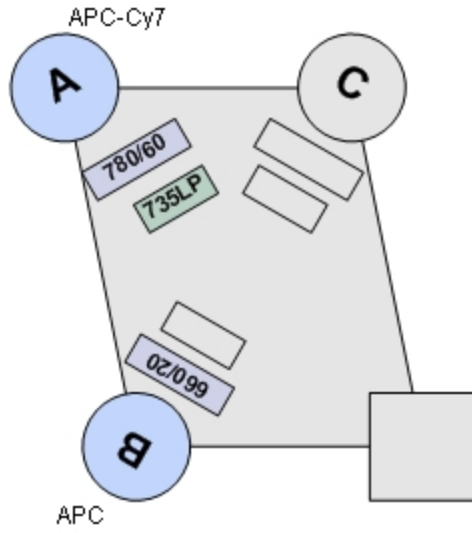

405nm Laser
(405nm)

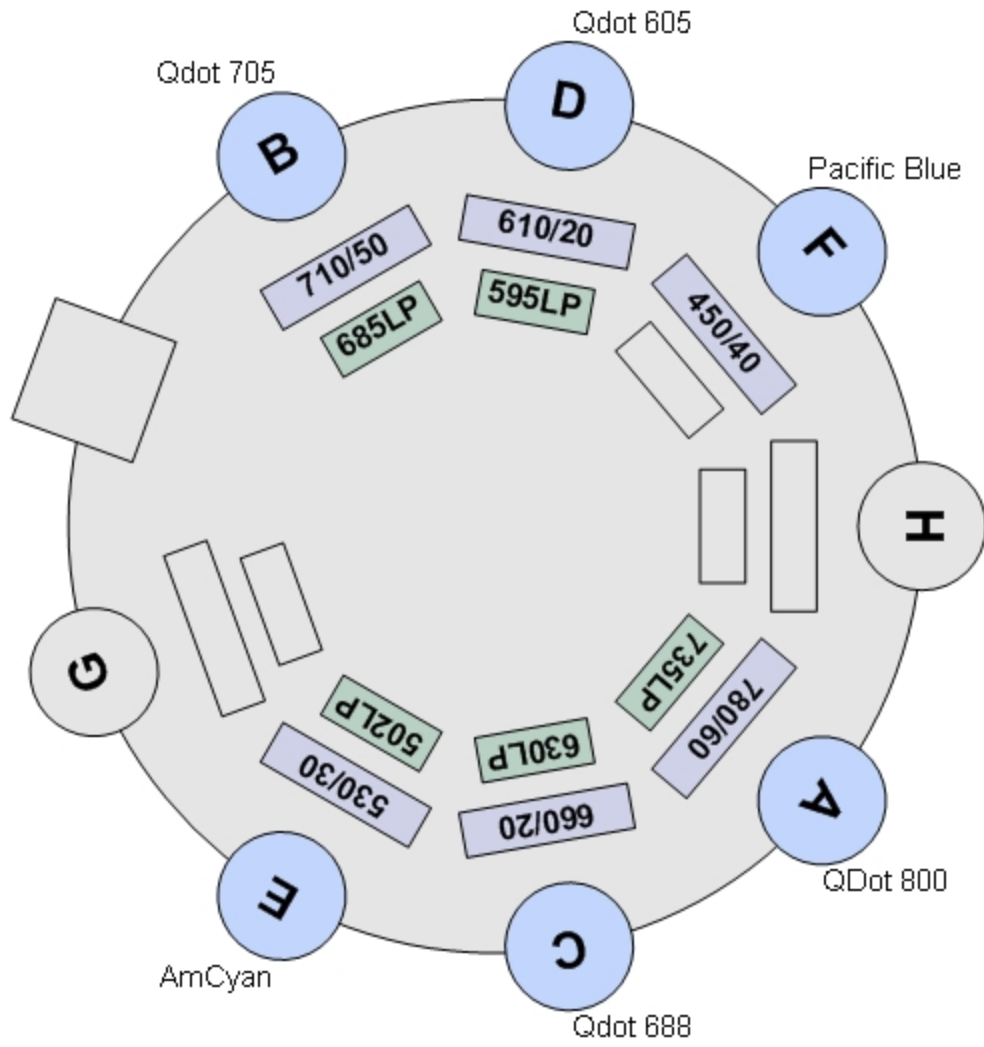

Comments: